
# JIR-301-M

# **Instruction Manual**



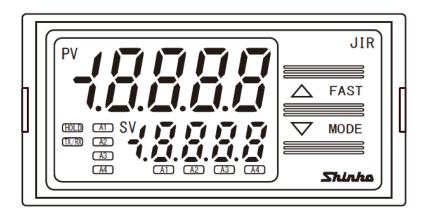

### **Preface**

Thank you for purchasing our Digital Indicator JIR-301-M. This manual contains instructions for the mounting, functions, operations and notes when operating the JIR-301-M. To prevent accidents arising from the misuse of this instrument, please ensure the operator receives this manual.

#### **Notes**

- This instrument should be used in accordance with the specifications described in the manual. If it is not used according to the specifications, it may malfunction or cause a fire.
- Be sure to follow the warnings, cautions and notices. If they are not observed, serious injury or malfunction may occur.
- The contents of this instruction manual are subject to change without notice.
- Care has been taken to ensure that the contents of this instruction manual are correct, but if there are any doubts, mistakes or questions, please inform our sales department.
- This instrument is designed to be installed through a control panel indoors. If it is not, measures must be taken to ensure that the operator cannot touch power terminals or other high voltage sections.
- Any unauthorized transfer or copying of this document, in part or in whole, is prohibited.
- Shinko Technos Co., Ltd. is not liable for any damage or secondary damage(s) incurred as a result of using this product, including any indirect damage.

# Safety Precautions (Be sure to read these precautions before using our products.)

The safety precautions are classified into categories: "Warning" and "Caution". Depending on circumstances, procedures indicated by  $\triangle$  Caution may result in serious consequences, so be sure to follow the directions for usage.



Procedures which may lead to dangerous conditions and cause death or serious injury, if not carried out properly.



Procedures which may lead to dangerous conditions and cause superficial to medium injury or physical damage or may degrade or damage the product, if not carried out properly.

# **⚠** Warning

- To prevent an electrical shock or fire, only Shinko or other qualified service personnel may handle the inner assembly.
- To prevent an electrical shock, fire or damage to the instrument, parts replacement may only be undertaken by Shinko or other qualified service personnel.

# $\triangle$

# **Safety Precautions**

- To ensure safe and correct use, thoroughly read and understand this manual before using this instrument.
- This instrument is intended to be used for industrial machinery, machine tools and measuring equipment. Verify correct usage after purpose-of-use consultation with our agency or main office. (Never use this instrument for medical purposes with which human lives are involved.)
- External protection devices such as protective equipment against excessive temperature rise, etc. must be installed, as malfunction of this product could result in serious damage to the system or injury to personnel. Proper periodic maintenance is also required.
- This instrument must be used under the conditions and environment described in this manual. Shinko Technos
  Co., Ltd. does not accept liability for any injury, loss of life or damage occurring due to the instrument being used
  under conditions not otherwise stated in this manual.

### Warning on Model Label



# **Caution**

Failure to handle this instrument properly may result in minor or moderate injury or property damage due to fire, malfunction, malfunction, or electric shock. Please read this manual before using the product to ensure that you fully understand the product.

À

# **Caution with Respect to Export Trade Control Ordinance**

To avoid this instrument from being used as a component in, or as being utilized in the manufacture of weapons of mass destruction (i.e. military applications, military equipment, etc.), please investigate the end users and the final use of this instrument.

In the case of resale, ensure that this instrument is not illegally exported.

### **Precautions for Use**

#### 1. Installation Precautions



### **Caution**

This instrument is intended to be used under the following environmental conditions (IEC61010-1): Overvoltage category II, Pollution degree 2

Ensure the mounting location corresponds to the following conditions:

- A minimum of dust, and an absence of corrosive gases
- No flammable, explosive gases
- · No mechanical vibrations or shocks
- No exposure to direct sunlight, an ambient temperature of 0 to 50°C (32 to 122°F) that does not change rapidly, and no icing
- An ambient non-condensing humidity of 35 to 85 %RH
- No large capacity electromagnetic switches or cables through which large current is flowing
- No water, oil or chemicals or where the vapors of these substances can come into direct contact with the unit
- Please note that the ambient temperature of this unit not the ambient temperature of the control panel must not exceed 50°C (122°F) if mounted through the face of a control panel, otherwise the life of electronic components (especially electrolytic capacitors) may be shortened.

Note • Avoid setting this instrument directly on or near flammable material even though the case of this instrument is made of flame-resistant resin.

### 2. Wiring Precautions



### Caution

- Do not leave wire remnants in the instrument, as they could cause a fire or malfunction.
- The terminal block of this instrument is designed to be wired from the upper side. The lead wire must be inserted from the upper side of the terminal, and fastened with the terminal screw.
- Tighten the terminal screw using the specified torque. If excessive force is applied to the screw when tightening, the terminal screw or case may be damaged.
- Do not pull or bend the lead wire on the terminal side when wiring or after wiring, as it could cause malfunction.
- Use a thermocouple and compensating lead wire according to the sensor input specifications of this instrument.
- Use the 3-wire RTD according to the sensor input specifications of this instrument.
- This instrument does not have a built-in power switch, circuit breaker and fuse. It is necessary to install a-power switch, circuit breaker and fuse near the instrument.

(Recommended fuse: Time-lag fuse, rated voltage 250 V AC, rated current 2 A)

- For a 24 V AC/DC power source, do not confuse polarity when using direct current (DC).
- When using a relay contact output type, externally use a relay according to the capacity of the load to protect the built-in relay contact.
- When wiring, keep input wires (thermocouple, RTD, etc.) away from AC power sources or load wires.
- Do not apply a commercial power source to the sensor which is connected to the input terminal nor allow the power source to come into contact with the sensor.

### 3. Operation and Maintenance Precautions

# **⚠** Caution

- Do not touch live terminals. This may cause electrical shock or problems in operation.
- Turn the power supply to the instrument OFF before retightening the terminal or cleaning. Working on or touching the terminal with the power switched ON may result in severe injury or death due to electrical shock.
- Use a soft, dry cloth when cleaning the instrument.

  (Alcohol based substances may tarnish or deface the unit.)
- As the display section is vulnerable, be careful not to put pressure on, scratch or strike it with a hard object.

#### 4. Compliance with Safety Standards

# À

### Caution

- Always install the recommended fuse described in this manual externally.
- If the instrument is used in a manner not specified by the manufacturer, the protection provided by the instrument may be impaired.
- Use a device with reinforced insulation or double insulation for the external circuit connected to this product.
- When using this product as a UL certified product, use a power supply conforming to Class 2 or LIM for the external circuit connected to the product.

#### Characters used in this manual (: No character is indicated.)

Onlar dotter 5 doca 1	onaracters asea in this manual ( No character is indicated.)													
Indication	-¦		-	2	3	닉	5	5	77	8	3	Ĺ	F	
Number, °C/°F	-1	0	1	2	3	4	5	6	7	8	9	ပ္	${}^{\circ}\! F$	
Indication	R	Π	Ь	Ē	ď	Ε	F	- E	Н	-	IJ	E	L	)(
Alphabet	A	4	В	С	D	Е	F	G	Η	I	J	K	┙	М
Indication	C	0	P	9	_	7	!	Ц	R	ľ.	j	7	111	
Alphabet	Ν	0	Р	Q	R	S	Т	U	>	W	Х	Υ	Z	

# **Contents**

1. Model	6
1.1 Model	6
1.2 How to Read the Model Label	7
2. Name and Functions	8
3. Mounting to the Control Panel	9
3.1 Site Selection	9
3.2 External Dimensions (Scale: mm)	9
3.3 Panel Cutout (Scale: mm)	9
3.4 Mounting the Unit	10
4. Wiring	11
4.1 Terminal Arrangement	11
4.2 Lead Wire Solderless Terminal	12
4.3 When Using as a Current Loop Supply	12
5. Setup	13
5.1 Registering the Selected Item or Value	13
5.2 Alarm Setting Mode	14
5.3 Auxiliary Function Setting Mode 1	15
5.4 Auxiliary Function Setting Mode 2	
5.5 Maintenance Mode	
6. Operation	26
6.1 Operation	26
6.2 Switching SV Display Indication	26
6.3 How to Use the Alarm Output	
6.4 How to Use the Event Input Function	26
7. Alarm Action	
7.1 High Limit Alarm, Low Limit Alarm	27
7.2 A3 High/Low Limit Range Alarm Action	28
7.3 A4 High/Low Limit Range Alarm Action	28
8. Specifications	29
8.1 Standard Specifications	29
8.2 Optional Specifications	33
9. Troubleshooting	35
10. Character Table	37
10.1 Alarm Setting Mode	37
10.2 Auxiliary Function Setting Mode 1	
10.3 Auxiliary Function Setting Mode 2	
10.4 Maintenance Mode	
11 Key Operation Flowchart	43

#### 1. Model

#### 1.1 Model

JIR-301-M	□,		Series name: JIR-30	01-M (W96 x H48 x	x D110 mm)			
Input M			Multi-range (*1)					
D			100 to 240 V AC					
Power supply	1		24 V AC/DC (*2)	24 V AC/DC (*2)				
		A4	Alarm 4 output (*3)					
		C5	Serial communication	on (RS-485)(*4)				
		P24	Insulated power out	put 24±3 V DC (*	5), (*6)			
		P5	Insulated power out	put 5±0.5 V DC (*	5), (*6)			
		DSB	Power for 2-wire train	nsmitter (Current l	oop supply)(*6), (*7)			
		TA2 (4-20)		Direct current	4 to 20 mA DC			
		TA2 (0-20)		output	0 to 20 mA DC			
			Transmission		0 to 1 V DC			
		TV2 (0-5)	output 2 (*3)	DC voltage	0 to 5 V DC			
Option		TV2 (1-5)		output	1 to 5 V DC			
		TV2 (0-10)			0 to 10 V DC			
		TA (0-20)		Direct current	0 to 20 mA DC			
			Lloor appoified	output				
		TV (0-1)	User specified Transmission		0 to 1 V DC			
		TV (0-5)	output (*8)	DC voltage	0 to 5 V DC			
		TV (1-5)		output	1 to 5 V DC			
		TV (0-10)			0 to 10 V DC			
		BK	Color: Black					
		TC	Terminal cover					


Alarms A1, A2 and A3 outputs are standard features. Alarm types (4 types for A1, A2, and 5 types for A3 as well as No alarm action) and Energized/De-energized can be selected.

- (\*1) Thermocouple (10 types), RTD (2 types), Direct current (2 types) and DC voltage (4 types) can be selected by keypad.
- (\*2) Power supply voltage 100 to 240 V AC is standard. When ordering 24 V AC/DC, enter '1' after the input code.
- (\*3) Alarm 4 output (A4 option) and Transmission output 2 (T□2 option) cannot be used together.
- (\*4) If Serial communication (RS-485)[C5 option] is ordered, the Event input function will not be available.
- (\*5) Insulated power output (P24 option) and Insulated power output (P5 option) cannot be used together. If Insulated power output (P24 option) or Insulated power output (P5 option) is ordered, A2 output cannot be used.
- (\*6) Insulated power output (P24 or P5 option) cannot be used with the Power for 2-wire transmitter (DSB option).
- (\*7) If Power for 2-wire transmitter (DSB option) is ordered, only 4 to 20 mA DC input (Built-in 50  $\,\Omega$  shunt resistor) can be used.
- (\*8) TA (4-20 mA DC) is a standard feature.

#### 1.2 How to Read the Model Label

Model labels are attached to the case and the inner assembly.


#### Top of the case

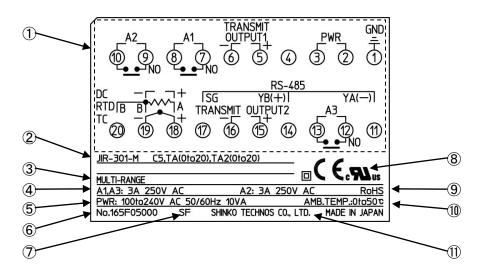

(Fig. 1.2-1)


No.	Description	Example
1	Terminal arrangement	Terminal arrangement of JIR-301-M
		C5, TA(0 to 20), TA2(0 to 20)
2	Model	JIR-301-M C5, TA(0 to 20), TA2(0 to 20)
3	Input	MULTI-RANGE (Multi-range input)
4	A1, A2, A3, A4, P24, P5 outputs	A1, A3: 3 A 250 V AC
		A2: 3 A 250 V AC
<b>⑤</b>	Power supply voltage	100 to 240 V AC 50/60 Hz,
	Power consumption	10 VA
6	Serial number	No.165F05000
7	Manufacturing factory ID	SF (Fukuoka factory)
8	Compliant standards	CE, UL
9	RoHS	RoHS directive compliant
10	Ambient temperature	0 to 50°C
11)	Manufacturer	SHINKO TECHNOS CO., LTD.

#### Inner assembly



No. Description		Example
1	Model	JIR-301-M
2	Serial number	No. 165F05000

# 2. Name and Functions

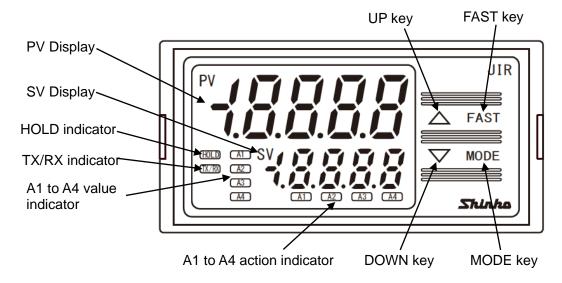

(Fig. 2-1)

#### Display, Indicator

Name	Description
PV Display	Indicates PV (process variable) or characters in the setting mode with the red LED.
SV Display	Indicates A1/A2/A3/A4 value or the set value in the setting mode with the green LED.
HOLD indicator	When PV is held (HOLD, Peak HOLD, Bottom HOLD), the yellow LED is lit.
TX/RX indicator	The yellow LED is lit during Serial communication (C5 option) TX (transmitting) output.
A1 value indicator	When A1 value is indicated on the SV Display, the green LED is lit.
A2 value indicator	When A2 value is indicated on the SV Display, the green LED is lit.
A3 value indicator	When A3 value is indicated on the SV Display, the green LED is lit.
A4 value indicator	When A4 value is indicated on the SV Display, the green LED is lit. (A4 option)
A1 action indicator	When A1 output is ON, the red LED is lit. While A1 output is held (maintained), the red LED flashes.
A2 action indicator	When A2 output is ON, the red LED is lit. While A2 output is held (maintained), the red LED flashes.
A3 action indicator	When A3 output is ON, the red LED is lit. While A3 output is held (maintained), the red LED flashes.
A4 action indicator	When A4 output is ON, the red LED is lit. While A4 output is held (maintained), the red LED flashes. (A4 option)

#### Key

Name	Description
UP key	Increases the numeric value.
	If High/Low limit range alarm is selected in [A4 type], and if the SV Display
	indicates A4 value, the SV Display indicates A4 high limit value while the UP key is
	pressed.
FAST key	Makes the set value change faster while pressing the UP/DOWN key and FAST
	key together.
DOWN key	Decreases the numeric value.
MODE key	Selects the setting mode, and registers the set value.



# Notice

When setting the specifications and functions of this instrument, connect mains power cable to terminals 2 and 3 first, then set them referring to "5. Setup" before performing "3. Mounting to the Control Panel" and "4. Wiring".

# 3. Mounting to the Control Panel


#### 3.1 Site Selection

This instrument is intended to be used under the following environmental conditions (IEC61010-1): Overvoltage category II, Pollution degree 2

Ensure the mounting location corresponds to the following conditions:

- A minimum of dust, and an absence of corrosive gases
- · No flammable, explosive gases
- · No mechanical vibrations or shocks
- No exposure to direct sunlight, an ambient temperature of 0 to 50°C (32 to 122°F) that does not change rapidly
- An ambient non-condensing humidity of 35 to 85 %RH
- No large capacity electromagnetic switches or cables through which large current is flowing
- No water, oil or chemicals or where the vapors of these substances can come into direct contact with the unit
- Please note that the ambient temperature of this unit not the ambient temperature of the control panel must not exceed 50°C (122°F) if mounted through the face of a control panel, otherwise the life of electronic components (especially electrolytic capacitors) may be shortened.


#### 3.2 External Dimensions (Scale: mm)

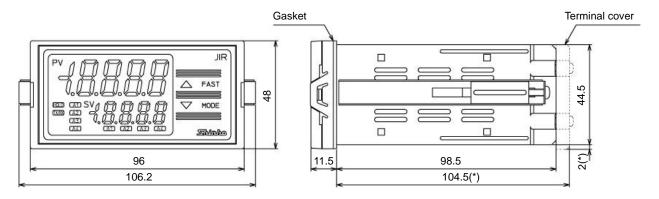

(\*) When terminal cover is used

(Fig. 3.2-1)

#### 3.3 Panel Cutout (Scale: mm)

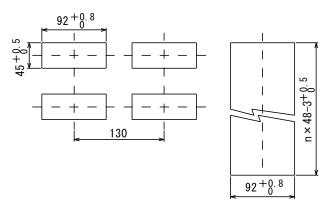

Vertical close mounting n: Number of mounted units

⚠ Caution: If vertical close mounting is used for the instrument, IP66 (Drip-proof/ Dust-proof) may be compromised, and all warranties will be invalidated.


(Fig. 3.3-1)

#### 3.4 Mounting the Unit

Mount the instrument vertically to the flat, rigid panel to ensure it adheres to the Drip-proof/Dust-proof specification (IP66).

Mountable panel thickness: 1 to 8 mm

- (1) Insert the instrument from the front side of the control panel.
- (2) Attach the mounting brackets by the slots on the right and left sides of the case, and secure the instrument in place with the screws.

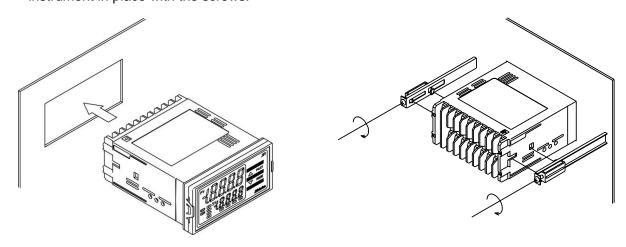

(Fig. 3.4-1)



# **Caution**

As the case of the JIR-301-M is made of resin, do not use excessive force while tightening screws, or the mounting brackets or case could be damaged.

0.12 N•m of torque is recommended.

# 4. Wiring


# Warning

Turn the power supply to the instrument off before wiring or checking. Working on or touching the terminal with the power switched on may result in severe injury or death due to electrical shock.

### Caution

- Do not leave wire remnants in the instrument, as they could cause a fire or malfunction.
- The terminal block of this instrument is designed to be wired from the upper side. The lead wire must be inserted from the upper side of the terminal, and fastened with the terminal screw.
- Tighten the terminal screw using the specified torque. If excessive force is applied to the screw when tightening, the terminal screw or case may be damaged.
- Do not pull or bend the lead wire on the terminal side when wiring or after wiring, as it could cause malfunction.
- Use a thermocouple and compensating lead wire according to the sensor input specifications of this instrument.
- Use the 3-wire RTD according to the sensor input specifications of this instrument.
- This instrument does not have a built-in power switch, circuit breaker and fuse. It is necessary to install a-power switch, circuit breaker and fuse near the instrument.
- (Recommended fuse: Time-lag fuse, rated voltage 250 V AC, rated current 2 A)
- For a 24 V AC/DC power source, do not confuse polarity when using direct current (DC).
- · When using a relay contact output type, externally use a relay according to the capacity of the load to protect the built-in relay contact.
- When wiring, keep input wires (thermocouple, RTD, etc.) away from AC power sources or load wires.
- Do not apply a commercial power source to the sensor which is connected to the input terminal nor allow the power source to come into contact with the sensor.

#### **4.1 Terminal Arrangement**

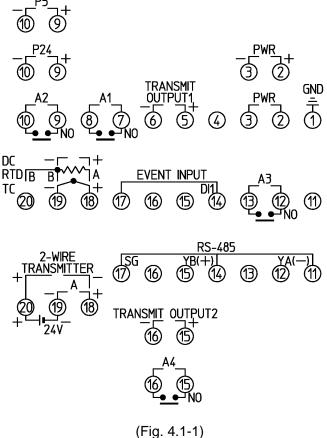


Terminal Name	Description
GND	Ground terminal
PWR	Power supply
TRANSMIT OUTPUT1	Transmission output 1
A1	A1 output
A2	A2 output
A3	A3 output
EVENT INPUT	Event input
TC	Thermocouple input
RTD	RTD input
DC	Direct current input, DC voltage input
	For Direct current input (externally mounted 50 $\Omega$ shunt resistor),
	connect a 50 $\Omega$ shunt resistor (sold separately) between input
	terminals.
P24	Insulated power output 24 V (P24 option)
P5	Insulated power output 5 V (P5 option)
RS-485	Serial communication (RS-485) (C5 option)
TRANSMIT OUTPUT2	Transmission output 2 (T□2 option)
A4	A4 output (A4 option)
Α	Direct current input (DSB option)
24V	Power for 2-wire transmitter (DSB option)

#### **4.2 Lead Wire Solderless Terminal**


Use a solderless terminal with an insulation sleeve in which an M3 screw fits as shown below. 0.63 N•m of torque is recommended.

Solderless Terminal	Manufacturer	Model
Y-type	NICHIFU TERMINAL INDUSTRIES CO., LTD.	TMEX1.25Y-3
	J.S.T.MFG.CO.,LTD.	VD1.25-B3A
Ring-type	NICHIFU TERMINAL INDUSTRIES CO., LTD.	TMEX1.25-3
	J.S.T.MFG.CO.,LTD.	V1.25-3



#### 4.3 When Using as a Current Loop Supply

Refer to the following wiring example.



(Fig. 4.3-1)

# 5. Setup

After power is turned ON, the input characters and temperature unit will be indicated on the PV Display, and the input range high limit (for thermocouple, RTD input) or scaling high limit (for Direct current, DC voltage input) will be indicated on the SV Display for approx. 3 sec. (Table 5-1)

During this time, all outputs and LED indicators are in an OFF status. Operation will then start, indicating the PV (process variable) on the PV Display, and A1, A2, A3 or A4 value on the SV Display.

(Table 5-1)

(10.010 0 1)	(Table 6-1)					
Sensor Input	PV Display (℃)	SV Display	PV Display (°F)	SV Display		
K	ETT	1370	EIIF	2500		
	E□ .C	4000	E□ F	7500		
J	JUL	1000	JEF	1800		
R	$r \square \mathcal{L}$	1750	r F	3200		
S	5 <u> </u>	1750	4 F	3200		
В	ЬШЕ	1820	ЬШЕ	3300		
E	ΕΠΕ	<u> 800</u>	EF	1500		
Т	Γ□ .Σ	4000	Γ□ .F	7500		
N	$\neg \square \mathcal{L}$	1300	n F	2300		
PL-∐	PL 25	1390	PL2F	2500		
C (W/Re5-26)	σΠΕ	23 15	<sub>⊆</sub> ∭F	4200		
Pt100	PC .E	8500	PT F	10000		
JPt100	JPT.E	5000	JPT.F	9000		
Pt100	PTUE	<u></u> 850	PT∐F	1500		
JPt100	JPCE	<u> </u>	JPCF	<u> </u>		
4-20 mA DC (*1)(*2)	420A					
0-20 mA DC (*1)(*2)	020R					
0-1 V DC (*1)	00 IB					
0-5 V DC (*1)	0 <u></u> 58	Scaling high				
1-5 V DC (*1)	<i>I</i> <u></u> 58	limit value				
0-10 V DC (*1)	0 108					
4-20 mA DC (*1)(*3)	4201					
0-20 mA DC (*1)(*3)	0201					

- (\*1) Input range and decimal point place can be selected.
- (\*2) Connect a 50  $\Omega$  shunt resistor (sold separately) between input terminals.
- (\*3) Has a built-in 50  $\Omega$  shunt resistor.

If Power for 2-wire transmitter (DSB option) is ordered, only 4 to 20 mA DC input (Built-in 50  $\Omega$  shunt resistor) can be used.

#### 5.1 Registering the Selected Item or Value

- To increase or decrease the numeric value, use the UP or DOWN key.
   To make the set value change faster, press the UP/DOWN key and FAST key together.
   Select an setting item with the UP or DOWN key.
- Register the setting item or value using the MODE key.

#### 5.2 Alarm Setting Mode

If the MODE key is pressed in PV/SV display mode, the unit will move to Alarm setting mode.

Character Factory Default	Setting Item, Function, Setting Range
R /	A1 value
	• Sets A1 output action point.
	Not available if No alarm action is selected in [A1 type]
	• Setting range: Refer to (Table 5.2-1).
82	A2 value
	Sets A2 output action point.
	Not available if No alarm action is selected in [A2 type]
	Not available if Insulated power output (P24 option or P5 option) is ordered.
	Setting range: Refer to (Table 5.2-1).
83	A3 value
	Sets A3 output action point.
	Not available if No alarm action or High/Low limit range alarm is selected in [A3 type]
	Setting range: Refer to (Table 5.2-1).
RY	A4 value
	Sets A4 output action point.
	Available when Alarm 4 output (A4 option) is ordered.
	Not available if No alarm action is selected in [A4 type]
	If High/Low limit range alarm is selected in [A4 type], A4 value matches A4 low limit
	alarm value.
	Setting range: Refer to (Table 5.2-1).
A4H	A4 high limit value
	Sets A4 output high limit action point.
	Available when Alarm 4 output (A4 option) is ordered, or when High/Low limit range
	alarm is selected in [A4 type].
	Setting range: Refer to (Table 5.2-1).

#### (Table 5.2-1)

(Table 3.2 T)	
Alarm Type	Setting Range
High limit alarm	Input range low limit to input range high limit (*1)
Low limit alarm	Input range low limit to input range high limit (*1)
High limit with standby alarm	Input range low limit to input range high limit (*1)
Low limit with standby alarm	Input range low limit to input range high limit (*1)
High/Low limit range alarm (A4)	A4 low limit value: Input range low limit (*2) to A4 high limit
	A4 high limit value: A4 low limit to input range high limit (*3)

- The placement of the decimal point follows the selection or input range.
- (\*1) For direct current and DC voltage input: Setting range is [Scaling low limit to Scaling high limit].
- (\*2) For direct current and DC voltage input: Will be substituted by the Scaling low limit.
- (\*3) For direct current and DC voltage input: Will be substituted by the Scaling high limit.

#### 5.3 Auxiliary Function Setting Mode 1

To enter Auxiliary Function Setting Mode 1, press and hold the **DOWN key** and **MODE key** (in that order) together for approx. 3 seconds in PV/SV Display Mode.

	ox. 3 seconds in PV/SV Display Mode.		
Character Factory Default	Setting Item, Function, Setting Range		
Lock	Set value lock		
	Locks the set values to prevent setting errors.		
	The setting item to be locked depends on the selection.		
	• (Unlock): All set values can be changed.		
	Lag (Lock 1): None of the set values can be changed.		
	$L_{QG} = \frac{1}{2}$ (Lock 2): Only Alarm setting mode (p.14) can be changed.		
	上ロロラ (Lock 3): All set values – except the input type (p.18) – can be changed.		
	However, changed values revert to their previous value after		
	power is turned off because they are not saved in the		
	non-volatile IC memory. Do not change any setting items in		
	Auxiliary function setting mode 2 (pp.18 - 24). If any item is		
	changed in Auxiliary function setting mode 2, it will affect the		
	alarm value (A1 value - A4 value).		
hat	Sensor correction coefficient		
(000	Sets sensor correction coefficient.		
	Sets slope of input value from a sensor.		
	PV after sensor correction= Current PV x (Sensor correction coefficient) +		
	(Sensor correction value)		
	Refer to 'Input Value Correction' (p. 17).		
	• Setting range: -10.000 to 10.000		
50	Sensor correction		
	This corrects the input value from the sensor.		
	When a sensor cannot be set at the exact location where measurement is desired, the		
	sensor-measured temperature may deviate from the temperature in the measurement		
	location. When using multiple indicators, sometimes the measured temperatures do		
	not match due to differences in sensor accuracy or installation site.		
	In such a case, the temperature in the installation site can be adjusted to the desired		
	temperature by adjusting the sensor input value.		
	PV after sensor correction= Current PV x (Sensor correction coefficient) +		
	(Sensor correction value)		
	Refer to 'Input Value Correction' (p.17).  • Setting range: -1000.0 to 1000.0°C (°F)		
	` ,		
	Direct current, DC voltage input: -10000 to 10000 (The placement of the decimal point follows the selection.)		
ENTL	Communication protocol		
nañL	Selects communication protocol.		
110116	Available only when Serial communication (C5 option) is ordered.		
	• กลูกี! : Shinko protocol		
	ਜ਼ਰੂਜਣ : Grimino protessor ਜ਼ਰੂਰੁਸ਼ : MODBUS ASCII mode		
	ਨਰੂਰਾ: MODBUS RTU mode		
	ងក្នុក្ស : Shinko protocol (Block Read/Write available)		
	ងក្នុងគឺ: MODBUS ASCII mode (Block Read/Write available)		
	๒๓๘๓ : MODBUS RTU mode (Block Read/Write available)		
	2.1.2		

Character Factory Default	Setting Item, Function, Setting Range		
cñno	Instrument number		
	• Sets the individual instrument number of this unit. (The instrument numbers should be set one by one when multiple instruments are connected in Serial communication.)		
	<ul> <li>Available only when the Serial communication (C5 option) is ordered</li> <li>Setting range: 0 to 95</li> </ul>		
cāhP	Communication speed		
95	Selects a communication speed equal to that of the host computer.		
	Available only when the Serial communication (C5 option) is ordered.		
	• □ 근' : 2400 bps		
	다. 역용 : 4800 bps		
	☐ 55 : 9600 bps		
	☐ /멸♂ : 19200 bps		
	☐∄84 : 38400 bps		
cñPr	Parity		
EBEn	Selects the parity.		
	Available when Serial communication (C5 option) is ordered, or when MODBUS ASCII mode or MODBUS RTU mode is selected in [Communication protocol].		
	• nonE : No parity		
	EHEn : Even		
	ಾರದ : Odd		
בהאר	Stop bit		
1	<ul><li>Selects the stop bit.</li><li>Available when Serial communication (C5 option) is ordered, or when MODBUS</li></ul>		
	ASCII mode or MODBUS RTU mode is selected in [Communication protocol].		
	•		

#### **Input Value Correction**

Input value can be corrected in [Sensor correction coefficient] and [Sensor correction] in Auxiliary Function Setting Mode 1.


In [Sensor correction coefficient], set the slope of temperature change.

In [Sensor correction], set the difference between temperatures before correction and after correction.

PV after input correction is expressed by the following formula.

PV after input correction = Current PV x Sensor correction coefficient + (Sensor correction value)

The following shows an example of input value correction using 'Sensor correction coefficient' and 'Sensor correction value'.

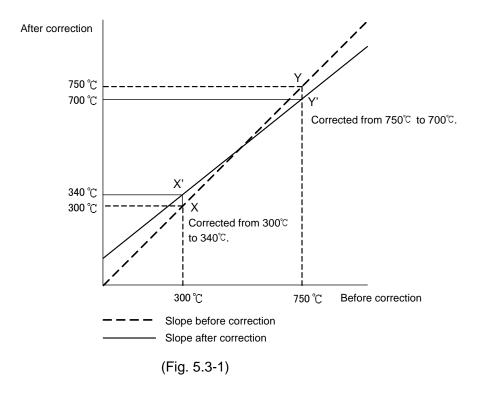

(1) Select any 2 points of PV to be corrected, and determine the PV after correction.

PV before correction: 300°C → PV after correction: 340°C

PV before correction: 750°C → PV after correction: 700°C

(2) Calculate Sensor correction coefficient from Step (1).

$$(Y'-X')/(Y-X) = (700-340)/(750-300) = 0.8$$

- (3) Enter a PV value of 300°C using an mV generator or dial resistor.
- (4) Set Step (2) value as a Sensor correction coefficient.
- (5) Read the PV.

240°C will be indicated.

- (6) Calculate the sensor correction value.
  - Calculate the difference between 'PV after correction' and Step (5) PV.

$$340^{\circ}\text{C} - 240^{\circ}\text{C} = 100^{\circ}\text{C}$$

- (7) Set Step (6) value as a Sensor correction value.
- (8) Enter an electromotive force or resistance value equivalent to 750℃ using an mV generator or dial resistor.
- (9) Read the PV, and confirm that 700°C is indicated.

#### **5.4 Auxiliary Function Setting Mode 2**

To enter Auxiliary Function Setting Mode 2, press and hold the **UP**, **DOWN** and **MODE keys** (in that order) together for approx. 3 seconds in PV/SV Display Mode.

Character	. 3 seconds in PV/SV Display Mode.			
Factory Default	Setting Item, Function, Setting Range			
≒Επ5 ±ΞΞΕ	<ul> <li>Input type</li> <li>The input type can be selected from thermocouple (10 types), RTD (2 types), Direct current (2 types) and DC voltage (4 types), and the unit °C/°F can be selected as well.</li> <li>Not available when Power for 2-wire transmitter (DSB option) is ordered.</li> <li>When changing the input from DC voltage to other inputs, remove the sensor connected to this instrument first, then change the input. If the input is changed with the sensor connected, the input circuit may break.</li> </ul>			
	(Table 5.4-1)  Character	Input Range	Character	Input Range
	ELL	K -200 to 1370℃	E F	K -320 to 2500°F
	E .C	K -200.0 to 400.0℃	E F	K -200.0 to 750.0°F
	J E	J -200 to 1000℃	J	J -320 to 1800° <sub>F</sub>
	- E	R 0 to 1760℃	-IIF	R 0 to 3200°F
	5 E	S 0 to 1760℃	4 F	S 0 to 3200°F
	b E	B 0 to 1820℃	b F	B 0 to 3300°F
	ELL	E -200 to 800℃	EIF	E -320 to 1500°F
	Ι Γ	T -200.0 to 400.0℃	Γ□ .F	T -200.0 to 750.0°F
		N -200 to 1300°C	n F	N -320 to 2300°F
	PL 2C	PL-	PL 2F	PL-
	ΕΞΕ	C(W/Re5-26) 0 to 2315℃		C(W/Re5-26) 0 to 4200°F
	PF E	Pt100 -200.0 to 850.0°C	•	Pt100 -200.0 to 1000.0°F
	JPF.E	JPt100 -200.0 to 500.0°C	_ •	JPt100 -200.0 to 900.0 F
	PEEE JPEE	Pt100 -200 to 850℃ JPt100 -200 to 500℃	PC_F JPCF	Pt100 -300 to 1500°F  JPt100 -300 to 900°F
	420A	4 to 20 mA DC -2000 to		3F(100 -300 to 900 F
	75 07	(Externally mounted 50 S		or)
	0208	0 to 20 mA DC -2000 to		,
		(Externally mounted 50 S		or)
	<u>                                    </u>	0 to 1 V DC -2000 to 10		
	0058	0 to 5 V DC -2000 to 10		
	1058	1 to 5 V DC -2000 to 10		
	4201 4201	0 to 10 V DC -2000 to 1 4 to 20 mA DC -2000 to		n 50 O shunt resister)
	0201			
		0 10 20 1114 00 -2000 10	TOOOO (Dant-I	11 30 St Stiditt (ESIStOI)
45 <u>L</u> H	Scaling high limit			
10000	Sets scaling high limit value.			
	Available when direct current or DC voltage input is selected in [Input type].			
	Setting range: Scaling low limit to Input range high limit (The placement of the			•
4566	decimal point follows the selection or input range.)  Scaling low limit			iput range.)
-2000	_	low limit value.		
	<ul> <li>Available when direct current or DC voltage input is selected in [Input type].</li> <li>Setting range: Input range low limit to Scaling high limit (The placement of the</li> </ul>			elected in [Input type].
		decimal point follows the	selection or in	put range.)

Character	Setting Item, Function, Setting Range		
Factory Default			
dP =	Decimal point place		
	Selects decimal point place.		
	Available when direct current or DC voltage input is selected in [Input type].		
	• III II: No decimal point		
	☐☐☐☐ : 1 digit after decimal point		
	☐☐☐☐ : 2 digits after decimal point		
	☐☐☐☐ : 3 digits after decimal point		
FILT	PV filter time constant		
	Sets PV filter time constant.		
	If the value is set too large, it affects alarm action due to the delay of response.		
	Setting range: 0.0 to 10.0 sec		
RL IF	A1 type		
	Selects an A1 type. See Section 7.1 (p.27).		
	• If A1 type is changed, A1 value will default to 0 (0.0).		
	•: No alarm action		
	High limit alarm		
	L Low limit alarm		
	H :: i High limit with standby alarm		
	L Low limit with standby alarm		
RL2F	A2 type		
	Selects an A2 type. See Section 7.1 (p.27).		
	Not available if Insulated power output (P24 option or P5 option) is ordered.		
	• If A2 type is changed, A2 value will default to 0 (0.0).		
	•: No alarm action		
	Harm: High limit alarm		
	L Low limit alarm		
	$H \square \square \bar{\omega}$ : High limit with standby alarm		
	L Low limit with standby alarm		
RL 3F	A3 type		
	Selects an A3 type. See Section 7.1 (p.27).		
	• If A3 type is changed, A3 value will default to 0 (0.0).		
	•: No alarm action		
	HIII : High limit alarm		
	L Low limit alarm		
	H□□□ : High limit with standby alarm		
	L Low limit with standby alarm		
	፲/ ⊿□ : High/Low limit range alarm [See Section 7.2 (p.28).]		

Character	Setting Item, Function, Setting Range		
Factory Default			
RL 4F 	A4 type		
	Selects an A4 type. See Section 7.1 (p.27).  Available when Alarm 4 output (A4 ention) is ordered.		
	Available when Alarm 4 output (A4 option) is ordered.		
	• If A4 type is changed, A4 value will default to 0 (0.0).		
	•: No alarm action		
	Hillinit alarm		
	Low limit alarm		
	Hamie: High limit with standby alarm		
	ட்ட பி. Low limit with standby alarm [See Section 7.3 (p.28).]		
R ILĀ	A1 Energized/De-energized		
nonL	Selects A1 Energized/De-energized.		
	Not available if No alarm action is selected in [A1 type].		
	When [A1 Energized] is selected, A1 output (terminals 7, 8) is conducted (ON)		
	while A1 action indicator is lit.		
	A1 output is not conducted (OFF) while A1 action indicator is unlit.		
	When [A1 De-energized] is selected, A1 output (terminals 7, 8) is not conducted		
	(OFF) while A1 action indicator is lit.		
	A1 output is conducted (ON) while A1 action indicator is unlit.		
	AA autout will be autout allow AO AO and A autout		
	A1 output will be substituted by A2, A3 or A4 output.		
	A1 output terminals will be substituted by A2, A3 or A4 output terminals as follows.		
	A2 output terminals: 9, 10		
	A3 output terminals: 12, 13		
	A4 output terminals: 15, 16		
	High limit alarm (Energized) High limit alarm (De-energized)		
	A1 hysteresis A1 hysteresis		
	<b>→</b>		
	ON ON		
	OFF — OFF — U		
	A1 value A1 value		
	(Fig. 5.4-1) (Fig. 5.4-2)		
	• ngāĻ: Energized		
	- E 出っ: De-energized		
R2LA	A2 Energized/De-energized		
noñL	Selects A2 Energized/De-energized.		
	Not available if No alarm action is selected in [A2 type].		
	Not available if Insulated power output (P24 option or P5 option) is ordered.		
	• ngni : Energized		
	ー ミピッ: De-energized		
83LA	A3 Energized/De-energized		
nañL	Selects A3 Energized/De-energized.		
_	Not available if No alarm action or High/Low limit range alarm is selected		
	in [A3 type].		
	• npnL : Energized		
	- 돈님与 : De-energized		

Character	Setting Item, Function, Setting Range	
Factory Default	octaing items, runotions, octaing items	
R4L5	A4 Energized/De-energized	
noñL	Selects A4 Energized/De-energized.	
	Available only when Alarm 4 output (A4 option) is ordered.	
	Not available if No alarm action is selected in [A4 type].	
	• nank : Energized	
<b>-</b>	구 돈 남 ' : De-energized	
A IHA	A1 hysteresis	
□□□ tØ	Sets A1 hysteresis.	
	Not available if No alarm action is selected in [A1 type].	
	• Setting range: 0.1 to 100.0°C (°F)	
	Direct current, DC voltage input: 1 to 1000 (The placement of the decimal point follows the selection.)	
R2HY	A2 hysteresis	
□□ iØ	Sets A2 hysteresis.	
	Not available if No alarm action is selected in [A2 type].	
	Not available if Insulated power output (P24 option or P5 option) is ordered.	
	• Setting range: 0.1 to 100.0℃ (℉)	
	Direct current, DC voltage input: 1 to 1000 (The placement of the decimal point follows the selection.)	
A3HY	A3 hysteresis	
III IØ	Sets A3 hysteresis.	
	Not available if No alarm action or High/Low limit range alarm is selected	
	in [A3 type].	
	• Setting range: 0.1 to 100.0℃ (℉)	
	Direct current, DC voltage input: 1 to 1000 (The placement of the decimal point	
750	follows the selection.)	
RYHY	A4 hysteresis	
	Sets A4 hysteresis.	
	Available only when Alarm 4 output (A4 option) is ordered.	
	Not available if No alarm action is selected in [A4 type].	
	• Setting range: 0.1 to 100.0°C (°F)	
	Direct current, DC voltage input: 1 to 1000 (The placement of the decimal point follows the selection.)	
8 192	A1 delay time	
	Sets A1 action delay time.	
	When setting time has elapsed after the input enters the alarm output range, the	
	alarm is activated.	
	Not available if No alarm action is selected in [A1 type].	
	Setting range: 0 to 10000 seconds	
8548	A2 delay time	
	Sets A2 action delay time.	
	When setting time has elapsed after the input enters the alarm output range, the	
	alarm is activated.	
	Not available if No alarm action is selected in [A2 type].	
	Not available if the Insulated power output (P24 option or P5 option) is ordered.	
	Setting range: 0 to 10000 seconds	

Character Factory Default	Setting Item, Function, Setting Range		
R3dy	A3 delay time		
	Sets A3 action delay time.		
	When setting time has elapsed after the input enters the alarm output range, the		
	alarm is activated.		
		action or High/Low limit range alarm is selected in	
	[A3 type].		
	• Setting range: 0 to 10000	seconds	
8443	A4 delay time		
	Sets A4 action delay time.		
	When setting time has elap	psed after the input enters the alarm output range, the	
	alarm is activated.		
	Available when Alarm 4 out	tput (A4 option) is ordered.	
	Not available if No alarm a	ction is selected in [A4 type].	
	Setting range: 0 to 10000 s	seconds	
[F-H	Transmission output 1 hig		
1370	Sets the Transmission out	put 1 high limit value.	
	Standard		
		Equals 20 mA DC output.	
	Optional		
		Equals 20 mA DC output.	
		Equals 1 V DC output.	
		Equals 5 V DC output.	
	0-10 V DC	Equals 10 V DC output.	
	Setting range: Transmission output 1 low limit to Input range high limit (The		
		of the decimal point follows the selection or input range.)	
FrL	Transmission output 1 lov		
-200	Sets the Transmission out	put 1 low limit value.	
	Standard	Francis ArrA DO cutout	
		Equals 4 mA DC output.	
	Optional  0-20 mA DC	Favels 0 m A DC systems	
		Equals 0 mA DC output.	
	0-1 V DC, 0-5 V DC, 0-10 V DC	Equals 0 V DC output.	
		Equals 1 V DC output.	
		·	
	• Setting range: Input range low limit to Transmission output 1 high limit (The placement of the decimal point follows the selection or input range.)		
[FHZ	Transmission output 2 hig		
םר <i>בו</i>	Sets the Transmission output 2 high limit value.		
12.10	Available when Transmission output 2 (T = 2 option) is ordered.		
	4-20 mA DC Equals 20 mA DC output.		
		Equals 20 mA DC output.	
		Equals 1 V DC output.	
		Equals 5 V DC output.	
	· · · · · · · · · · · · · · · · · · ·	Equals 10 V DC output.	
		on output 2 low limit to Input range high limit (The	
	placement of the decimal point follows the selection or input range.)		

Character	Sotting Itom Function Sotting Pango		
Factory Default	Setting Item, Function, Setting Range		
r-L2	Transmission output 2 low limit		
-200	Sets the Transmission output 2 low limit value.		
		ion output 2 (T□2 option) is ordered.	
	4-20 mA DC	Equals 4 mA DC output.	
	0-20 mA DC	Equals 0 mA DC output.	
	0-1 V DC, 0-5 V DC,	Equals 0 V DC output.	
	0-10 V DC		
	1-5 V DC	Equals 1 V DC output.	
		e low limit to Transmission output 2 high limit (The	
	· ·	of the decimal point follows the selection or input range.)	
Hald	Event input function		
HoLd	Selects Event input function		
	• H□L ☐ (HOLD):	munication (C5 option) is ordered.	
	_ = = - , ,	held and indicated by closing Event input terminals (14,	
	_	is cancelled by opening the Event input terminals (14,	
	17). THE FIGED TURBLES 17).	1 is cancelled by opening the Event input terminals (14,	
	P_H (Peak HOLD):		
	1	PV is indicated by closing Event input terminals (14, 17).	
	·	on is cancelled by opening the Event input terminals	
	(14, 17).		
	<b>占_</b> H□ (Bottom HOLD):		
	The updated minimum PV is indicated by closing Event input terminals (14, 17).		
	The Bottom HOLD function is cancelled by opening Event input terminals		
	(14, 17).		
	片급 (Alarm HOLD 1):		
	If any of [A1 HOLD function] to [A4 HOLD function] is set to "Enabled", and if the		
	alarm is ON, the alarm will be maintained by closing Event input terminals (14,		
	17). The Alarm HOLD function will be cancelled by eneming Event input terminals.		
	The Alarm HOLD function will be cancelled by opening Event input terminals (14, 17). While the Event input terminals (14, 17) are open, the Alarm HOLD		
	function will be disabled		
	HL 글론 (Alarm HOLD 2):		
	1	ction] to [A4 HOLD function] is set to "Enabled", and if the	
	_ · ·	will be maintained by opening the Event input terminals	
	(14, 17).		
	The Alarm HOLD function	on will be cancelled by closing Event input terminals (14,	
	17). While the Event inp	out terminals (14, 17) are closed, the Alarm HOLD	
	function will be disabled		
R IHd	A1 HOLD function		
nonE	Enables/Disables the A1 HOLD function.		
	Not available if No alarm action is selected in [A1 type].		
		t to "Enabled", and if the alarm is ON, the alarm output	
		ned until the following is conducted.	
	• The power is turned O	sed for approx. 3 seconds.	
	· ·	d by the Event input function.	
	During A1 HOLD, the A1 a		
	• npnE : Disabled		
	HaLd : Enabled		

Character Factory Default	Setting Item, Function, Setting Range		
R2Hd	A2 HOLD function		
nonE	• Enables/Disables the A2 HOLD function.		
1121112	Not available if No alarm action is selected in [A2 type].		
	Not available if Insulated power output (P24 option or P5 option) is ordered.		
	• If A2 HOLD function is set to "Enabled", and if the alarm is ON, the alarm output		
	ON status will be maintained until the following is conducted.		
	The FAST key is pressed for approx. 3 seconds.		
	The power is turned OFF.		
	The HOLD is cancelled by the Event input function.		
	During A2 HOLD, the A2 action indicator flashes.		
	• ¬¬¬E: Disabled H¬Ld: Enabled		
R3Hd	A3 HOLD function		
nonE	Enables/Disables the A3 HOLD function.		
	Not available if No alarm action or High/Low limit range alarm is selected in [A3 type].		
	• If A3 HOLD function is set to "Enabled", and if the alarm is ON, the alarm output		
	ON status will be maintained until the following is conducted.		
	The FAST key is pressed for approx. 3 seconds.		
	The power is turned OFF.		
	The HOLD is cancelled by the Event input function.		
	During A3 HOLD, the A3 action indicator flashes.		
	• nanE: Disabled Hala: Enabled		
RYHd	A4 HOLD function		
nonE	• Enables/Disables the A4 HOLD function.		
	Available when Alarm 4 output (A4 option) is ordered.		
	Not available if No alarm action is selected in [A4 type].		
	• If A4 HOLD function is set to "Enabled", and if the alarm is ON, the alarm output		
	ON status will be maintained until the following is conducted.		
	The FAST key is pressed for approx. 3 seconds.     The power is turned OFF.		
	The HOLD is capselled by the Event input function.		
	<ul> <li>The HOLD is cancelled by the Event input function.</li> <li>During A4 HOLD, the A4 action indicator flashes.</li> </ul>		
	• nanE: Disabled Hald: Enabled		
roof	Square root function		
nonE	Enables/Disables the square root extraction function.		
TIGITIE	Indication value or square root extraction value is expressed by the formula below.		
	$PV' = \sqrt{PV}$		
	PV': Indication value, square root extraction value		
	PV: Process variable		
	・ロロロE: Disabled はら足に Enabled		
Leur	Low level cutoff (e.g.) Input: 4-20 mA DC, Scaling range: 0-100		
	Sets the low level cutoff value.  Low level cutoff: 1.0%		
	• When PV input is near 0 (zero),  In this case, PV becomes 0 if it is lower than 1.0%.		
	the result of square root extraction value		
	changes considerably with only		
	a very small change of input.		
	In this case, the PV is forced to		
	become 0 (zero).		
	If PV input is lower than the low level		
	cutoff value, the PV will become 0.		
	• Setting range: 0.0 to 25.0% of input		
	range 0 4 20 Input (mA)		
	(Fig. 5.4-3) 1.0% of input range (4.16 mA)		

#### **5.5 Maintenance Mode**

To enter Maintenance mode, press the **UP** and **FAST keys** (in that order) together for approx. 5 seconds in PV/SV Display Mode.

If the unit enters Maintenance mode, all outputs are forced to turn OFF.

Character Factory Default	Setting Item, Function, Setting Range		
A. R I	A1 output ON/OFF		
off	A1 output can be turned ON by the UP key, and OFF by the DOWN key.		
	• □FF□: Output OFF		
	gn : Output ON		
ALBS	A2 output ON/OFF		
oFF	A2 output can be turned ON by the UP key, and OFF by the DOWN key.		
	Not available if Insulated power output (P24 option or P5 option) is ordered.		
	□FF     Output OFF		
	□□: Output ON		
AER3	A3 output ON/OFF		
oFF.	A3 output can be turned ON by the UP key, and OFF by the DOWN key.		
	□FF     Output OFF		
	□□: Output ON		
A_RY	A4 output ON/OFF		
off[	A4 output can be turned ON by the UP key, and OFF by the DOWN key.		
	Available when Alarm 4 output (A4 option) is ordered.		
	• □FF□: Output OFF		
	□□: Output ON		
ĀT I	Transmission output 1 manual output		
	Sets output amount of Transmission output 1.		
	• Setting range: 0.0 to 100.0%		
AL L E	Transmission output 2 manual output		
	Sets output amount of Transmission output 2.		
	Available when Transmission output 2 (T □ 2 option) is ordered.		
	• Setting range: 0.0 to 100.0%		

# 6. Operation

#### 6.1 Operation

After the JIR-301-M is mounted to the control panel and wiring is completed, operate the unit following the procedure below.

(1) Turn the power supply to the JIR-301-M ON.

For approximate 3 sec after the power is switched ON, the input characters and the temperature unit are indicated on the PV Display, and input range high limit (thermocouple, RTD input) or scaling high limit (Direct current, DC voltage input) is indicated on the SV Display. See (Table 5-1) (p.13). During this time, all outputs and LED indicators are in an OFF status.

After that, Indication starts, indicating PV on the PV Display, and A1, A2, A3 or A4 value on the SV Display.

(2) Enter each set value.

Enter each set value, referring to Section "5. Setup".

#### 6.2 Switching SV Display Indication

To change indication on the SV Display, press the UP and MODE keys (in that order) together in the PV/SV Display Mode. The next alarm value (of the currently indicated A1-A4 value) will be displayed. If the UP and MODE keys (in that order) are pressed together at [A4 value indication], the unit reverts to [A1 value indication].

Indication	Setting Item, Function		
PV	A1 value indication		
A1 value	Indicates A1 value on the SV Display, and the A1 value indicator is lit.		
	Not available if No alarm action is selected in [A1 type].		
PV	A2 value indication		
A2 value	Indicates A2 value on the SV Display, and the A2 value indicator is lit.		
	Not available if No alarm action is selected in [A2 type].		
	Not available if Insulated power output (P24 option or P5 option) is ordered.		
PV	A3 value indication		
A3 value	Indicates A3 value on the SV Display, and the A3 value indicator is lit.		
	Not available if No alarm action or High/Low limit range alarm is selected in [A3 type].		
PV	A4 value indication		
A4 value	Indicates A4 value on the SV Display, and the A4 value indicator is lit.		
	If High/Low limit range alarm is selected in [A4 type], the SV Display indicates		
	A4 low limit value.		
	While the UP key is pressed, the SV Display indicates A4 high limit value.		
	Available when Alarm 4 output (A4 option) is ordered.		
	Not available if No alarm action is selected in [A4 type].		

#### **6.3 How to Use the Alarm Output**

- (e.g.) To use A1 output, follow the procedure below.
- (1) Select an A1 type in [A1 type] (p.19) in Auxiliary function setting mode 2.
- (2) Set the following items in Auxiliary function setting mode 2 if required: A1 Energized/De-energized (p.20), A1 hysteresis (p.21), A1 delay time (p.21), A1 HOLD function (p.23)
- (3) Set the A1 value in [A1 value (p.14)] in Alarm setting mode.

A1 output settings are complete.

The same applies to A2, A3 and A4 output.

#### 6.4 How to Use the Event Input Function

- (e.g.) To use Peak HOLD of the Event input function, follow the procedure below.
- (1) Select Peak HOLD in [Event input function (p.23)] in Auxiliary function setting mode 2.
- (2) The updated maximum PV is indicated by closing Event input terminals (14, 17). The Peak HOLD function is cancelled by opening Event input terminals (14, 17).

# 7. Alarm Action

#### 7.1 High Limit Alarm, Low Limit Alarm

	High limit alarm	Low limit alarm
A1 action	OFF A1 value	A1 hysteresis  ON  OFF  A1 value
A1 output		
	High limit with standby alarm	Low limit with standby alarm
A1 action	OFF A1 value	A1 hysteresis ON OFF A1 value
A1 output		

: A1 output terminals (7, 8) ON

: A1 output terminals (7, 8) ON or OFF

: A1 output terminals (7, 8) OFF

: A1 output is in standby.


• The following terminal numbers are used for respective alarm outputs.

A2 output terminals: 9, 10 A3 output terminals: 12, 13 A4 output terminals: 15, 16

• A1, A2, A3 or A4 action indicator is lit when each output terminals are ON.

A1, A2, A3 or A4 action indicator is turned off when its output terminals are OFF.

#### 7.2 A3 High/Low Limit Range Alarm Action

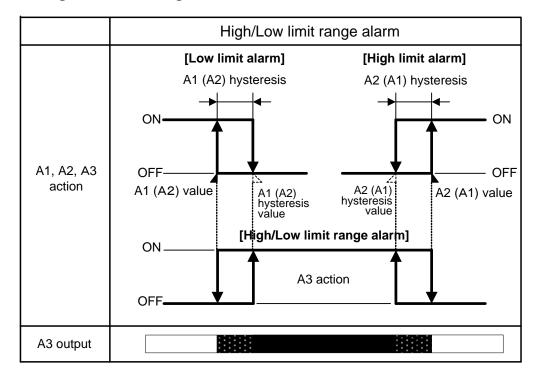

: A1 output terminals (7, 8): OFF, A2 output terminals (9, 10): OFF, A3 output terminals (12, 13): ON

: A1 output terminals (7, 8), A2 output terminals (9, 10) and A3 output terminals (12, 13): ON or OFF

: A1 output terminals (7, 8): ON, A2 output terminals (9, 10): ON, A3 output terminals (12, 13): OFF

A3 High/Low limit range alarm action is determined by setting A1 value and A2 value.


A3 is activated (ON) when both A1 and A2 are OFF – by combining A1 High limit alarm (or High limit with standby alarm) and A2 Low limit alarm (or Low limit with standby alarm) and vice versa. When standby function, hysteresis or delay time for A1 and A2 are set, check the below A3 action.

#### Please note the following:

- If A1 or A2 with standby alarm is selected, A3 is turned ON while A1 or A2 is in standby.
- If A1 or A2 hysteresis increases, A3 ON span decreases.
- When A1 or A2 delay time (setting time) increases, A3 ON time increases.
- If A1 or A2 delay time (setting time) is set, while A1 or A2 delay time is working (when power to the instrument is turned ON), A3 is turned ON.

#### 7.3 A4 High/Low Limit Range Alarm Action

When High/Low limit range alarm is selected in [A4 type]:

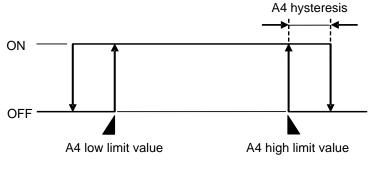

(Fig. 7.3-1)

# 8. Specifications

#### 8.1 Standard Specifications

Rating

Input	_						
	Thermo-	Thermo- K, J, R, S, B, E, T, N, PL-II, C(W/Re5-26)					
	couple						
	RTD						
		Allowable input lead wire resistance: 10 $\Omega$ max. per wire					
	Direct	0-20 mA DC, 4-20 mA DC (Select an externally mounted shunt resistor					
	current	or a built-	or a built-in shunt resistor.)				
		Input im	pedance: 50 $\Omega$				
		Allowabl	le input current: 50	mA DC max	<b>(</b> .		
	DC voltage	voltage 0-1 V DC					
		Input impedance: 1 M $\Omega$ min.					
		Allowabl	le input voltage: 5 V	DC max.			
		Allowable signal source resistance: 2 kΩ max. 0-5 V DC, 1-5 V DC, 0-10 V DC					
		Input impedance: 100 k $\Omega$ min. Allowable input voltage: 15 V DC max.					
		Allowable signal source resistance: 100 $\Omega$ max.					
Power							
supply	Model JIR-301-M JIR-301-M 1					01-M 1	
voltage	Power suppl	y voltage	100 to 240 V AC	50/60Hz	24 V AC/DC	50/60Hz	
	Allowable vo	ltage	85 to 264 V AC		20 to 28 V A0	C/DC	
	fluctuation ra	ange					

#### **General Structure**

Dimensions	96 x 48 x 110 mm (W x H x D)			
Mounting	Flush (Mountable panel thickness: 1 to 8 mm)			
Material	Case: Flame-resistant resin, Color: Light gray			
Drip-proof/Dust-proof	f IP66 (for front panel only)			
Setting method Input system using membrane sheet key				
Display PV Display: Red LED 5-digits, Character size, 16 x 7.2 mm (H x W)				
	SV Display: Green LED 5-digits, Character size, 10 x 4.8 mm (H x W)			

#### **Indication Performance**

Indication		
accuracy	Thermocouple	Within $\pm 0.2\%$ of each input span $\pm 1$ digit, or within $\pm 2^{\circ}\mathbb{C}$ ( $4^{\circ}\mathbb{F}$ ), whichever is greater However, R, S input, 0 to $200^{\circ}\mathbb{C}$ (32 to $392^{\circ}\mathbb{F}$ ): Within $\pm 6^{\circ}\mathbb{C}$ ( $12^{\circ}\mathbb{F}$ ) B input, 0 to $300^{\circ}\mathbb{C}$ (32 to $572^{\circ}\mathbb{F}$ ): Accuracy is not guaranteed. K, J, E, T, N input, Less than $0^{\circ}\mathbb{C}$ ( $32^{\circ}\mathbb{F}$ ): Within $\pm 0.4\%$ of each input span $\pm 1$ digit
RTD		Within ±0.1% of each input span±1 digit, or within ±1°C (2°F), Whichever is greater
	Direct current, DC voltage	Within ±0.2% of each input span ±1 digit
Input samp	ling period	125 ms

#### Standard Function

A1 output, A2 output, A3 output The alarm action point can be set at random (process alarm), and if the input reaches the randomly set action point, the alarm output turns ON or OFF corresponding to the alarm type and Energized/De-energized selection.

The alarm type can be selected from; No alarm action, High limit alarm, Low limit alarm, High limit with standby alarm, Low limit with standby alarm and High/Low limit range alarm (for A3 output only).

High/Low limit range alarm can be selected when A1 High limit alarm (High limit with standby alarm) and A2 Low limit alarm (Low limit with standby alarm) are combined, or when A1 Low limit alarm (Low limit with standby alarm) and A2 High limit alarm (High limit with standby alarm) are combined.


ingii mine alai	in (Fight little With Standby diarri) are combined.
Action	ON/OFF action
Hysteresis	0.1 to 100.0℃ (℉)
	Direct current, DC voltage input: 1 to 1000 (The placement of the
	decimal point follows the selection.)
Alarm	Enables/Disables the Alarm HOLD function.
HOLD	If Alarm HOLD function is set to "Enabled", and if the alarm is ON,
	the alarm output ON status will be maintained until the following is
function	conducted.
	The FAST key is pressed for approx. 3 seconds.
	The power is turned OFF.
	The HOLD is cancelled by the Event input function.
	During Alarm HOLD, corresponding alarm action indicator flashes.
Output	Relay contact 1a
·	Control capacity: 3 A 250 V AC (resistive load)
	Electrical life: 100,000 cycles

Transmission output 1

Converting the PV to analog signal every 125 ms, outputs the value in direct current. (Unaffected by the HOLD function) (When using the Transmission output 1 value as an input for other instruments, check that the input impedance of these instruments is smaller than the maximum load resistance of Transmission output 1.)

Resolution	12000
Direct current	4 to 20 mA DC (Load resistance: Max. 550 Ω)
Output accuracy	Within ±0.3% of transmission output span
Response time	400 ms+ Input sampling period (0%→90%)

#### **Insulation, Dielectric Strength**

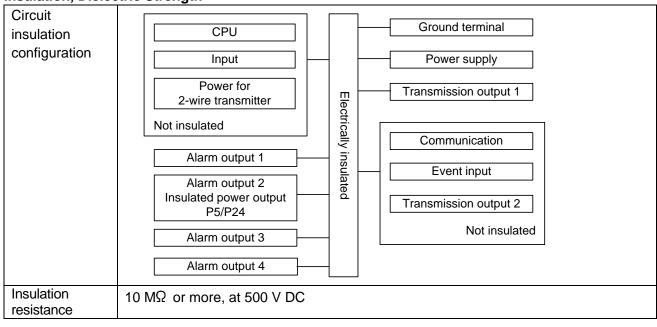

Dielectric	Input terminal and ground terminal: 1.5 kV AC for 1 minute
strength	Input terminal and power terminal: 1.5 kV AC for 1 minute
0	Power terminal and ground terminal: 1.5 kV AC for 1 minute
	Output terminal and ground terminal: 1.5 kV AC for 1 minute
	Output terminal and power terminal: 1.5 kV AC for 1 minute
	(Output terminals: A1, A2, A3 and A4 output terminals, Transmission output 1
	terminals, Transmission output 2 terminals and communication terminals)

#### **Attached Function**

Burnout

Input error				
indication	Indication	Contents		
	flashes.	Overscale: Measured value has exceeded indication range high limit.		
	flashes.	Underscale: Measured value has dropped below indication range low limit.		

When the thermocouple or RTD input is burnt out, the PV Display flashes \_\_\_\_\_.

• Thermocouple, RTD input

Input	Input Range	Indication Ran	
	-200 to 1370°C	-250 to 1420°C	
<	-320 to 2500°F	-420 to 2600°F	
`	-200.0 to 400.0℃	-200.0 to 450.0℃	
	-200.0 to 750.0°F	-200.0 to 850.0°F	
l	-200 to 1000°C	-250 to 1050°C	
	-320 to 1800°F	-420 to 1900°F	
1	0 to 1760°C	-50 to 1810°C	
₹	0 to 3200 F	-100 to 3300°F	
}	0 to 1760°C	-50 to 1810°C	
	0 to 3200 F	-100 to 3300°F	
<b>.</b>	0 to 1820°C	-50 to 1870°C	
	0 to 3300°F	-100 to 3400°F	
	-200 to 800°C	-250 to 850°C	
	-320 to 1500°F	-420 to 1600°F	
	-200.0 to 400.0℃	-200.0 to 450.0℃	
	-200.0 to 750.0°F	-200.0 to 850.0°F	
	-200 to 1300°C	-250 to 1350°C	
	-320 to 2300°F	-420 to 2400°F	
L- II	0 to 1390°C	-50 to 1440°C	
<b>∟-</b> Π	0 to 2500°F	-100 to 2600°F	
(\M/DoE 26\	0 to 2315°C	-50 to 2365°C	
(W/Re5-26)	0 to 4200 F	-100 to 4300°F	
	-200.0 to 850.0℃	-200.0 to 900.0℃	
t100	-200.0 to 1000.0°F	-200.0 to 1100.0°F	
1100	-200 to 850°C	-210 to 900°C	
	-300 to 1500°F	-318 to 1600°F	
· · · · · · · · · · · · · · · · · · ·	-200.0 to 500.0℃	-200.0 to 550.0℃	
Pt100	-200.0 to 900.0°F	-200.0 to 1000.0°F	
-1100	-200 to 500°C	-207 to 550°C	
	-300 to 900°F	-312 to 1000°F	

Input error	• Direct current	DC voltage input			
indication	Direct current, DC voltage input  If measured value exceeds Indication range high limit value, the PV Display				
Indication	flashes, and if measured value drops below the Indication range low limit				
		splay flashes			
	Indication range: [Scaling low limit value – Scaling span x 1%] to				
	[Scaling high limit value + Scaling span x 10%]				
	DC input disconnection:  When DC input is disconnected, the PV Display flashes for 4 to 20 mA DC				
	and 1 to 5 V DC input, and for 0 to 1 V DC input.  For 0 to 20 mA DC, 0 to 5 V DC and 0 to 10 V DC input, the PV Display indicates				
	the value corresponding with 0 mA or 0 V.				
Set value lock		ues to prevent setting errors. (p.15)			
Sensor correction		it value from a sensor.			
coefficient	Coto ciopo di ilipo	a value from a concen.			
Sensor correction	Corrects the input	value from a sensor. (p.15)			
Power failure		s backed up in the non-volatile IC memory.			
countermeasure	•	·			
Self-diagnosis		tored by a watchdog timer, and if an abnormal status is found on			
		-301-M is switched to warm-up status.			
Automatic cold	This detects the temperature at the connecting terminal between the thermocouple and				
junction temp.	the instrument, and always maintains it at the same status as if the reference junction				
compensation	·	ure was at 0°C (32°F).			
Event input	-	out function from 3 types of HOLD function and 2 types of Alarm			
function	HOLD function. Not available if Serial communication (C5 option) is ordered.				
	HOLD	PV (indicated value only) at the given time is held and			
		indicated by closing Event input terminals (14, 17). The HOLD			
		function is cancelled by opening Event input terminals (14, 17).			
	Peak HOLD	The updated maximum PV is indicated by closing Event input			
		terminals (14, 17). The Peak HOLD function is cancelled by			
		opening Event input terminals (14, 17).			
	Bottom HOLD	The updated minimum PV is indicated by closing Event input			
		terminals (14, 17). The Bottom HOLD function is cancelled by			
		opening Event input terminals (14, 17).			
	Alarm HOLD 1	If any of [A1 HOLD function] to [A4 HOLD function] is set to			
		"Enabled", and if the alarm is ON, the alarm will be maintained			
		by closing Event input terminals (14, 17).			
		The alarm HOLD function will be cancelled by opening Event			
		input terminals (14, 17). While Event input terminals (14, 17)			
		are open, the alarm HOLD function will be disabled.			
	Alarm HOLD 2	If any of [A1 HOLD function] to [A4 HOLD function] is set to			
		"Enabled", and if the alarm is ON, the alarm will be maintained			
		by opening Event input terminals (14, 17).			
		The alarm HOLD function will be cancelled by closing Event			
		input terminals (14, 17). While Event input terminals (14, 17)			
		are closed, the alarm HOLD function will be disabled.			
107	A440 m 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0	ON the input sharesters and terresters with the input sharesters.			
Warm-up	•	ned ON, the input characters and temperature unit will be indicated			
indication	on the PV Display, and the input range high limit (for thermocouple, RTD input) or scaling high limit (for direct current, DC voltage input) will be indicated on the SV				
	Display for approx. 3 sec.				
	bispiay ioi appio	A. U 350.			

#### Other

Power			
consumption	Supply Voltage Power Consumption		
	100 to 240 V AC	Approx. 8 VA (When maximum options are ordered: Approx.10 VA)	
	24 V AC	Approx. 6 VA (When maximum options are ordered: Approx.9 VA)	
	24 V DC	Approx. 4 W (When maximum options are ordered: Approx.7 W)	
Ambient temperature	0 to 50°C (32 to 122°F)		
Ambient humidity	35 to 85 %RH (non-condensing)		
Altitude	2,000 m or less		
Weight	Approx. 300 g		
Accessories	Screw type mounting brackets (1 set), Instruction manual excerpt (1 copy),		
	Unit label (1 label), Terminal cover (1 piece, When the TC option is ordered)		

#### 8.

Serial	When the C5 option is ordered, the Event input function cannot be used.						
communication	The following operations can be carried out from an external computer.						
(C5 option)	<ul> <li>Reading and setting</li> </ul>	g of various	set values				
	Reading of PV and action status						
	• Function change						
	Communication line	EIAF	S-485				
	Communication method	Half-	uplex communication				
	Communication speed	2400	4800, 9600, 19200, 38	400 bps			
	Synchronization meth	od Start-	stop synchronization				
	Parity	Even	Odd , No parity (Select	table by keypad)			
	Stop bit	1, 2 (	Selectable by keypad)				
	Communication protocol	In ad	Shinko protocol, MODBUS ASCII, MODBUS RTU In addition, each protocol above is available with Block Read/Write.				
		(Sele	(Selectable by keypad)				
	Connectable number of units	er Maxii	Maximum 31 units to 1 host computer  Double detection by parity and checksum				
	Communication error detection	Doub					
	Data format						
	Communication protocol	Shin proto		CII MODBUS RTU			
	Start bit	1	1	1			
	Data bit (*1)	7	7	8			
	Parity	Even	Selection [Even] (*2)	Selection [No parity] (*2)			
	Stop bit	1	Selection [1] (*2)	Selection [1] (*2)			
	(*1) Data bit is automatically selected upon selecting the communication protocol. (*2) [ ]: Basic set value						
Alarm 4 output	This option and Transmission output 2 (T□2 option) cannot be used together.						
(A4 option)	Alarm type, alarm action and alarm output are the same as those of A1, A2 and						
, ,	output except High/L			,			

Insulated power	If this option is o	rdered t	he A2 function will be disabled.			
output	This option cannot be used with the Insulated power output (P5 option) together,					
(P24 option)	or cannot be used with Power for 2-wire transmitter (DSB option) together.					
(1 2 1 6 5 1.01.)	Output voltage		24±3 V DC (When load current is 30 mA)			
	Ripple voltage		Within 200 mV DC (When load current is 30 mA)			
	Max load current		30 mA DC			
Insulated power	If this option is o	rdered, t	he A2 function will be disabled.			
output	This option cann	ot be us	ed with the Insulated power output (P24 option) together,			
(P5 option)	or cannot be use	ed with P	ower for 2-wire transmitter (DSB option) together.			
	Output voltage		5±0.5 V DC (When load current is 30 mA)			
	Ripple voltage		Within 200 mV DC (When load current is 30 mA)			
	Max load curre	nt	30 mA DC			
Power for	If this option is o	ordered, o	only 4 to 20 mA DC input (Built-in 50 Ω shunt resistor)			
2-wire	can be used.					
transmitter	•		ed with the Insulated power output (P24 option or P5			
(DSB option)	option) together.					
	Output voltage		24±3 V DC (When load current is 30 mA)			
	Ripple voltage		Within 200 mV DC (When load current is 30 mA)			
	Max load curre	nt	30 mA DC			
Transmission	· ·	ot be us	t be used with Alarm 4 output (A4 option) together.			
output 2	Resolution		12000			
(T□2 option)	Output accuracy		Within ±0.3% of transmission output span			
	Response time		400 ms + Input sampling period (0%→90%)			
	Option Code		Transmission Output Type			
	TA2 (4-20)	Direct	4 to 20 mA DC (Load resistance: Max 550 Ω)			
	TA2 (0-20)	current	`			
	TV2 (0-1)	Garrona	0 to 1 V DC (Load resistance: Minimum 100 k $\Omega$ )			
	TV2 (0-5)	DC	0 to 5 V DC (Load resistance: Minimum 500 k $\Omega$ )			
	TV2 (1-5)	voltage	· · · · · · · · · · · · · · · · · · ·			
	TV2 (0-10)	Tonago	0 to 10 V DC (Load resistance: Minimum 1 $M\Omega$ )			
	(0 . 0)	<u> </u>	1 0 10 1 DO (2000 TOOLOGITOO, TAIRITTION T WILL)			
User specified	Standard Transr	nission o	utput can be changed to the following 'User specified			
Transmission	Transmission ou	ıtput'.				
output	<b>Option Code</b>		Transmission Output Type			
(TA, TV option)	TA (0-20)	Direct current	0 to 20 mA DC (Load resistance: Max 550 $\Omega$ )			
	TV (0-1)		0 to 1 V DC (Load resistance: Minimum 100 kΩ)			
	TV (0-5)	DC	0 to 5 V DC (Load resistance: Minimum 500 kΩ)			
	TV (1-5)	voltage	,			
	TV (0-10)		0 to 10 V DC (Load resistance: Minimum 1 MΩ)			
Color Black	Panel: Dark gray					
(BK option)	Case: Black					
\	Odoc. Didok					
Terminal cover		protectio	n terminal cover			

# 9. Troubleshooting

If any malfunctions occur, refer to the following items after checking that power is being supplied to the JIR-301-M.

Problem	Possible Cause	Solution
The PV Display	Internal memory is defective.	Contact us or our agency in your region.
indicates Err 1.		
The PV Display indicates	Burnout of thermocouple, RTD or disconnection of DC voltage (0 to 1 V DC)	Replace each sensor.  How to check whether the sensor is burnt out [Thermocouple]  If the input terminals of the instrument are shorted, and if a value around room temperature is indicated, the instrument is likely to be operating normally, however, the sensor may be burnt out.  [RTD]  If approx. 100 Ω of resistance is connected to the input terminals between A-B of the instrument and between B-B is shorted, and if a value around 0°C (32°F) is indicated, the instrument is likely to be operating normally, however, the sensor may be burnt out.  [DC voltage (0 to 1 V DC)]  If the input terminals of the instrument are shorted, and if a scaling low limit value is indicated, the
	Check whether the input terminals of thermocouple,	instrument is likely to be operating normally, however, the signal wire may be disconnected.  Connect the sensor terminals to the instrument input terminals securely.
The DV District	RTD or DC voltage (0 to 1 V DC) are securely connected to the instrument input terminals.	
The PV Display flashes	Check whether input signal wire for DC voltage (1 to 5 V DC) or direct current (4 to 20 mA DC) is disconnected.	How to check whether the input signal wire is disconnected [DC voltage (1 to 5 V DC)]  If the input to the input terminals of the instrument is 1 V DC and if a scaling low limit value is indicated, the instrument is likely to be operating normally, however, the signal wire may be disconnected.  [Direct current (4 to 20 mA DC)]  If the input to the input terminals of the instrument is 4 mA DC and if a scaling low limit value is indicated, the instrument is likely to be operating normally, however, the signal wire may be disconnected.
	Check whether input signal wire for DC voltage (1 to 5 V DC) or direct current (4 to 20 mA DC) is securely connected to the instrument input terminals.	Ensure that the input signal wire is securely connected to the instrument input terminals.
	Check if polarity of thermocouple or compensating lead wire is correct. Check whether codes (A, B, B) of RTD agree with the instrument terminals.	Wire them correctly.

Problem	Possible Cause	Solution
The PV Display	Check whether the input signal	How to check whether the input signal wire is
keeps indicating	wires of DC voltage (0 to 5 V	disconnected
the value set in	DC, 0 to 10 V DC) and direct	[DC voltage (0 to 5 V DC, 0 to 10 V DC)]
[Scaling low limit].	current (0 to 20 mA DC) is	If the input to the input terminal of this instrument
	disconnected.	is 1 V DC, and if a value (converted value from
		scaling high, low limit setting) corresponding to 1
		V DC is indicated, the instrument is likely to be
		operating normally, however, the input signal wire
		may be disconnected.
		[Direct current (0 to 20 mA DC)]
		If the input to the input terminal of this instrument
		is 4 mA DC, and if a value (converted value from
		scaling high, low limit setting) corresponding to 4
		mA DC is indicated, the instrument is likely to be
		operating normally, however, the input signal wire
	Objectively at hearth and hearth and	may be disconnected.
	Check whether the input	Connect the input terminals of DC voltage and
	terminals of DC voltage	current to the input terminals of this instrument
	(0 to 5 V DC, 0 to 10 V DC) or	securely.
	direct current (0 to 20 mA DC) are securely connected to the	
	instrument input terminals.	
The indication of	Check whether sensor input or	Select the sensor input and temperature unit (°C
PV Display is	temperature unit (°C or °F) is	or °F) correctly.
irregular or	correct.	
unstable.	Sensor correction coefficient or	Set them to suitable values.
	Sensor correction value is	
	unsuitable.	
	Check whether the sensor	Use a sensor with appropriate specifications.
	specification is correct.	
	AC leaks into the sensor	Use an ungrounded type sensor.
	circuit.	
	There may be equipment that	Keep the instrument clear of any potentially
	interferes with or makes noise	disruptive equipment.
	near the instrument.	
Values on the PV	Terminals 14 and 17 are	Cancel the HOLD function by opening terminals
Display do not	closed, and the HOLD function	14 and 17.
change.	is working.	
Even if the UP key	Set value lock (Lock 1 or	Release the lock in [Set value lock].
or DOWN key is	Lock 2) is selected.	
pressed, values		
do not change.		

# 10. Character Table

Depending on the model and setting contents, some setting items do not appear.

#### 10.1 Alarm Setting Mode

If the MODE key is pressed in PV/SV Display Mode, the unit will move to Alarm setting mode.

Character	Sotting Itom Function Sotting Pango	
Factory Default	Setting Item, Function, Setting Range	
R I	A1 value	
	Refer to (Table 10.1-1).	
R2	A2 value	
	Refer to (Table 10.1-1).	
R3	A3 value	
	Refer to (Table 10.1-1).	
RH	A4 value	
	Refer to (Table 10.1-1).	
R4H	A4 high limit value	
	Refer to (Table 10.1-1).	

#### (Table 10.1-1)

Alarm Type	Setting Range
High limit alarm	Input range low limit to input range high limit (*1)
Low limit alarm	Input range low limit to input range high limit (*1)
High limit with standby	Input range low limit to input range high limit (*1)
alarm	
Low limit with standby	Input range low limit to input range high limit (*1)
alarm	
High/Low limit range	A4 low limit value: Input range low limit (*2) to A4 high limit
alarm (A4)	A4 high limit value: A4 low limit to input range high limit (*3)

<sup>•</sup> The placement of the decimal point follows the selection or input range.

<sup>(\*1)</sup> For direct current and DC voltage input: Setting range is [Scaling low limit to Scaling high limit].

<sup>(\*2)</sup> For direct current and DC voltage input: Will be substituted by the Scaling low limit.

<sup>(\*3)</sup> For direct current and DC voltage input: Will be substituted by the Scaling high limit.

#### 10.2 Auxiliary Function Setting Mode 1

To enter Auxiliary Function Setting Mode 1, press and hold the DOWN key and MODE key (in that order) together for approx. 3 seconds in PV/SV Display Mode.

	x. 3 seconds in PV/SV Display Mode.	
Character	Setting Item, Function, Setting Range	
Factory Default		
Lock	Set value lock	
	<ul> <li> (Unlock): All set values can be changed.</li> </ul>	
	Lac! (Lock 1): None of the set values can be changed.	
	'- ਕੁਟ ਤੂੰ (Lock 2): Only Alarm setting mode (p.14) can be changed.	
	になる。 (Lock 3): All set values – except the input type (p.18) – can be changed.	
	However, changed values revert to their previous value after	
	power is turned off because they are not saved in the	
	non-volatile IC memory. Do not change any setting items in	
	Auxiliary function setting mode 2 (pp.18 - 24). If any item is	
	changed in Auxiliary function setting mode 2, it will affect the	
A ANGEL	alarm value (A1 value - A4 value).	
50E	Sensor correction coefficient	
1000	• Setting range: -10.000 to 10.000	
5 <u>0</u>	Sensor correction	
	• Setting range: -1000.0 to 1000.0℃ (℉)	
	Direct current, DC voltage input: -10000 to 10000 (The placement of the decimal	
	point follows the selection.)	
EAHL	Communication protocol	
noñL	• กอกี <u>!</u> : Shinko protocol	
	ក៏ក្នុដ់ក៏ : MODBUS ASCII mode	
	កិត្តdr : MODBUS RTU mode	
	๒๓๑ีL: Shinko protocol (Block Read/Write available)	
	ភ្ក៨ឱ: MODBUS ASCII mode (Block Read/Write available)	
	៦ភ៨r : MODBUS RTU mode (Block Read/Write available)	
cñno	Instrument number	
□□□ Ø	Setting range: 0 to 95	
cāhP	Communication speed	
<b>98</b>	• ፲근거: 2400 bps	
	☐ 남용: 4800 bps	
	□□写長:9600 bps	
	୍ର /ସ∄: 19200 bps	
	୍ର∃ <i>ଞ୍ଜ</i> : 38400 bps	
cñPr	Parity	
EBEn	• ¬¬¬E : No parity	
	트님트교 : Even	
	ದರ⊡: Odd	
ะกั <b>ว</b> โ	Stop bit	
	• [ ] ; 1 bit	

#### 10.3 Auxiliary Function Setting Mode 2

To enter Auxiliary Function Setting Mode 2, press and hold the UP, DOWN and MODE keys (in that order) together for approx. 3 seconds in PV/SV Display Mode.

Character	Setting Item, Function, Setting Range			
Factory Default	Setting item, Function, Setting Kange			
5En5	Input type			
E	(Table 10.3-1)			
	Character	Input Range	Character	Input Range
	EUE	K -200 to 1370°C	EF	K -320 to 2500°F
	LE□ .E	K -200.0 to 400.0℃	E□ F	K -200.0 to 750.0° <sub>F</sub>
	JIII	J -200 to 1000℃	J∏F	J -320 to 1800°F
	- Ε	R 0 to 1760°C	r F	R 0 to 3200°F
	5 E	S 0 to 1760℃	'-	S 0 to 3200°F
	ЬШЕ	B 0 to 1820℃	b F	B 0 to 3300°F
	ELLE	E -200 to 800°C	EIF	E -320 to 1500°F
	Γ□ .Ε	T -200.0 to 400.0℃	Γ□ .F	T -200.0 to 750.0°F
	η L	N -200 to 1300℃	n F	N -320 to 2300°F
	PL 25	PL-	PL2F	PL-
	ΕΠΕ	C(W/Re5-26) 0 to 2315℃	c F	C(W/Re5-26) 0 to 4200°F
	<i>PF .</i> [	Pt100 -200.0 to 850.0℃	PT F	Pt100 -200.0 to 1000.0°F
	JPT.E	JPt100 -200.0 to 500.0℃	JPT.F	JPt100 -200.0 to 900.0°F
	Prut	Pt100 -200 to 850℃	PTUF	Pt100 -300 to 1500°F
	UPT [	JPt100 -200 to 500℃	JPFF	JPt100 -300 to 900°F
	420A	4-20 mA DC -2000 to 100	000 (Externally	mounted 50 $\Omega$ shunt resistor)
	020A	0-20 mA DC -2000 to 100	000 (Externally	mounted 50 $\Omega$ shunt resistor)
	BO 18	0-1 V DC -2000 to 1000	0	
	005H	0-5 V DC -2000 to 1000	0	
	/ <u></u> 58	1-5 V DC -2000 to 1000	0	
	0 108	0-10 V DC -2000 to 100	00	
	4201	4-20 mA DC -2000 to 10	0000 (Built-in 5	50 Ω shunt resistor)
	8281	0-20 mA DC -2000 to 10	0000 (Built-in 5	50 Ω shunt resistor)
SELH	Soaling high	limit		
10000 10000	Scaling high limit  • Setting range: Scaling low limit to Input range high limit (*)			
\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\\	Scaling low li	· ·	inge mgm minit	( )
-2000		: Input range low limit to Sca	iling high limit (	(*)
3P 3	Decimal poin			\ /
	-	decimal point		
		digit after decimal point		
	☐☐☐☐ : 2 digits after decimal point			
	<u> </u>	digits after decimal point		
FILT	PV filter time constant			
00	<ul> <li>Setting range</li> </ul>	e: 0.0 to 10.0 sec		
AL IF	A1 type			
		alarm action		
	High limit alarm			
	L□□□: Low limit alarm H□□□ : High limit with standby alarm			
	_	n iimit with standby alarm  / limit with standby alarm		
	I .	point follows the coloction of		

<sup>(\*)</sup> The placement of the decimal point follows the selection or input range.

Characters, Factory Default	Setting Item, Function, Setting Range	
RL 2F	A2 type	
	• : No alarm action	
	High limit alarm	
	L Low limit alarm	
	H □ Ū : High limit with standby alarm	
	L . Low limit with standby alarm	
AL 3F	A3 type	
	• : No alarm action	
	H∷∷∷: High limit alarm	
	と回回: Low limit alarm	
	H□□□ : High limit with standby alarm	
	L	
	፲; ៨☐: High/Low limit range alarm	
RL YF	A4 type	
	•: No alarm action	
	Harring: High limit alarm	
	L Low limit alarm	
	H□□ū : High limit with standby alarm	
	L .: Low limit with standby alarm	
	፲ੵ੶ 님igh/Low limit range alarm	
A ILA	A1 Energized/De-energized	
noñL	• កក្ករ៉ុ : Energized	
	卢돈분특: De-energized	
R2LA	A2 Energized/De-energized	
noñL	• nant: Energized	
	උ도남与 : De-energized	
R3Lā	A3 Energized/De-energized	
noñL	• nañl: Energized	
	ー E 出っ: De-energized	
RYLA	A4 Energized/De-energized	
noñL	・ ヮヮ゙゙た: Energized ァミガウ: De-energized	
Ti nui		
A IHY	A1 hysteresis • Setting range: 0.1 to 100.0℃ (℉)	
III ιΩ	\ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \	
82HY	Direct current, DC voltage input: 1 to 1000 (*)  A2 hysteresis	
mens   III lO	• Setting range: 0.1 to 100.0℃ (℉)	
	Direct current, DC voltage input: 1 to 1000 (*)	
R3HY	A3 hysteresis	
	• Setting range: 0.1 to 100.0℃ (℉)	
	Direct current, DC voltage input: 1 to 1000 (*)	
RYHY	A4 hysteresis	
	• Setting range: 0.1 to 100.0℃ (℉)	
11.1 <b>4.2</b>	Direct current, DC voltage input: 1 to 1000 (*)	
	zos. canoni, zo ronago input. 1 to 1000 ( )	

<sup>(\*)</sup> The placement of the decimal point follows the selection.

Characters, Factory Default	Setting Item, Function, Setting Range
R IdY	A1 delay time
	Setting range: 0 to 10000 seconds
824Y	A2 delay time
$\Box\Box$	Setting range: 0 to 10000 seconds
8389	A3 delay time
	Setting range: 0 to 10000 seconds
RYdY	A4 delay time
	Setting range: 0 to 10000 seconds
F-H I	Transmission output 1 high limit
1370	Setting range: Transmission output 1 low limit to Input range high limit (*)
T-L1	Transmission output 1 low limit
-200	Setting range: Input range low limit to Transmission output 1 high limit (*)
[-H2	Transmission output 2 high limit
1370	Setting range: Transmission output 2 low limit to Input range high limit (*)
T-L2	Transmission output 2 low limit
-200	Setting range: Input range low limit to Transmission output 2 high limit (*)
HoLd	Event input function
HoLd	・ HロL d (HOLD):
	PV at the given time is held and indicated by closing Event input terminals (14,
	17). The HOLD function is cancelled by opening Event input terminals (14, 17).
	P_H□ (Peak HOLD):
	The updated maximum PV is indicated by closing Event input terminals (14, 17).
	The Peak HOLD function is cancelled by opening Event input terminals (14, 17).
	<ul><li>½ H□ (Bottom HOLD):</li><li>The updated minimum PV is indicated by closing Event input terminals (14, 17).</li></ul>
	The Bottom HOLD function is cancelled by opening Event input terminals (14, 17).
	17).
	/   서도급 : (Alarm HOLD 1):
	If any of [A1 HOLD function] to [A4 HOLD function] is set to "Enabled", and if the
	alarm is ON, the alarm will be maintained by closing Event input terminals (14,
	17).
	The alarm HOLD function will be cancelled by opening Event input terminals
	(14, 17). While the Event input terminals (14, 17) are open, the alarm HOLD
	function will be disabled.
	HL 님은 (Alarm HOLD 2):
	If any of [A1 HOLD function] to [A4 HOLD function] is set to "Enabled", and if the
	alarm is ON, the alarm will be maintained by opening Event input terminals (14, 17).
	The alarm HOLD function will be cancelled by closing Event input terminals
	(14, 17). While the Event input terminals (14, 17) are closed, the alarm HOLD
	function will be disabled.
A IHA	A1 HOLD function
nonE	• ngnE : Disabled
1000	Hala : Enabled
	TIGE S. ENGOIGE

<sup>(\*)</sup> The placement of the decimal point follows the selection or input range.

Characters, Factory Default	Setting Item, Function, Setting Range
R2Hd	A2 HOLD function
nonE	• nanE : Disabled
	HaL님 : Enabled
R3Hd	A3 HOLD function
nonE	• nanE : Disabled
	HaL님 : Enabled
RYHd	A4 HOLD function
nonE	• nanE : Disabled
	HaLd : Enabled
roof	Square root function
nonE	• ngnE : Disabled
	나누톤 : Enabled
LELIT	Low level cutoff
□□ UΩ	Setting range: 0.0 to 25.0% of input range


#### **10.4 Maintenance Mode**

To enter Maintenance mode, press the UP and FAST keys (in that order) together for approx. 5 seconds in PV/SV Display Mode.

If the unit enters Maintenance mode, all outputs are forced to turn OFF.

Characters, Factory Default	Setting Item, Function	
⊼⊑R I	A1 output ON/OFF	
oFF.	• □FF□ : Output OFF	
	ਰੁਸ਼∷∷: Output ON	
AER2	A2 output ON/OFF	
oFF.	• □FF : Output OFF	
	ធ្វក : Output ON	
AER3	A3 output ON/OFF	
oFF.	• □FF : Output OFF	
	□□□ : Output ON	
A_RY	A4 output ON/OFF	
oFF.	□FF     : Output OFF	
	□□□□□□□□□□□□□□□□□□□□□□□□□□□□□□□□□□□□□	
ALT 1	Transmission output 1 manual output	
	• Setting range: 0.0 to 100.0%	
ALT 2	Transmission output 2 manual output	
	• Setting range: 0.0 to 100.0%	

# 11. Key Operation Flowchart

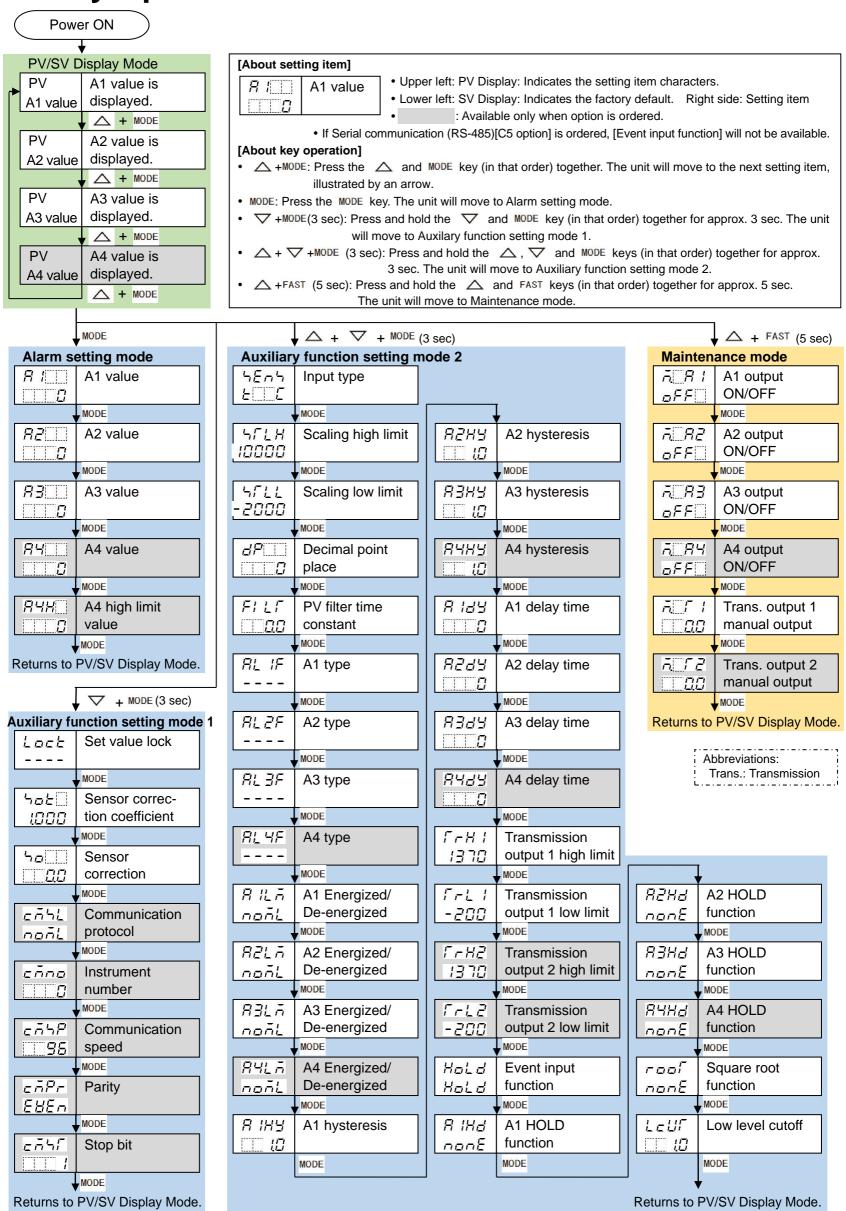

For any inquiries about this unit, please contact our agency or the vendor where you purchased the unit. Please provide your model and serial number.

(e.g.)

- Model ----- JIR-301-M
- Serial number ---- No. 165F05000

In addition to the above, please let us know the details of the malfunction, or discrepancy, and the operating conditions.